

warranty details

Your Drive branded product is warranted to be free of defects in materials and workmanship for one year from date of purchase.

This device was built to exacting standards and carefully inspected prior to shipment. This warranty is an expression of our confidence in the materials and workmanship of our products and our assurance to the customer.

In the event of a defect covered by this warranty, we will at our option supply parts or replace the device.

This warranty does not cover device failure due to owner misuse or negligence, or normal wear and tear. The warranty does not extend to non-durable components, such as rubber accessories, castors and grips, which are subject to normal wear and need periodic replacement.

If you have any queries or require full warranty conditions, please contact your Drive stockist.

It is recommended that the rollator is serviced on an annual basis, if the rollator is used by a single user. If the rollator is used in a multi-user environment (such as in communal housing) servicing may be required more frequently. Any servicing, maintenance or repairs should be done by competent personnel such as a Drive Medical dealer.



Drive Medical Ltd
Ainley's Industrial Estate, Elland,
West Yorkshire, GB Hx5 9JP
www.drivemedical.co.uk

Doc code: WA018_IFU (Iss 11/14)

x-fold rollator



www.drivemedical.co.uk

safety procedures

1. Make sure the rollator is fully opened, the seat is down and the frame is locked securely.
2. Ensure that hand grips are at equal heights. Test the rollator for stability before applying full weight to hand grips.
3. Ensure that good health and safety practice is used for carrying and lifting items, such as the rollator.
4. Always lock the brakes before sitting and do not use seat when on a gradient or uneven ground.
5. Replace the tyres when significantly worn or damaged.
6. For your health and comfort, make sure that you adopt a comfortable posture and that you can operate the brakings with ease. Check the brakes function correctly (i.e. Stop the rear wheels from turning when the brakes are applied.)
7. Do not exceed the maximum weight limit of 135kg (21 stone).
8. Ensure the backrest is firmly secured before using. Check that both screws are securely tightened before use.

specification

Overall dimensions (cm):	68 (L) x 64 (W) x 81 - 94 (H)
Seat dimensions (cm) :	23 (L) x 46 (W) x 56 (H)
Overall dimensions (in):	27"(L) x 25"(W) x 32" - 37"(H)
Seat dimensions (in):	9" (L) x 18" (W) x 22" (H)
Weight:	7.5kg (17lb)
Weight Limit:	135kg (21 stone)



Handle Height Adjustment

To adjust the handle height, push the brass button and raise or lower the handle until it is locked at the desired height. Ensure both handles are set to the same height.

care and maintenance

Ensure the walker is used only as an aid for mobility.

Ensure the walker is kept clean. Wipe down the walker with a damp cloth on a regular basis.


Check the moving parts (e.g. wheels and height adjustment) regularly. All moving parts should operate freely without excessive movement or play.

Ensure that the hand operated cable brakes are functioning correctly. When squeezed or locked on, the two rear wheels should not be able to turn.

All the fasteners (screws, nuts and bolts) are to be checked regularly to ensure they are securely tightened.

Check that the front castor wheel(s) swivels freely. Withdraw the walker from use if it does not.

parts description

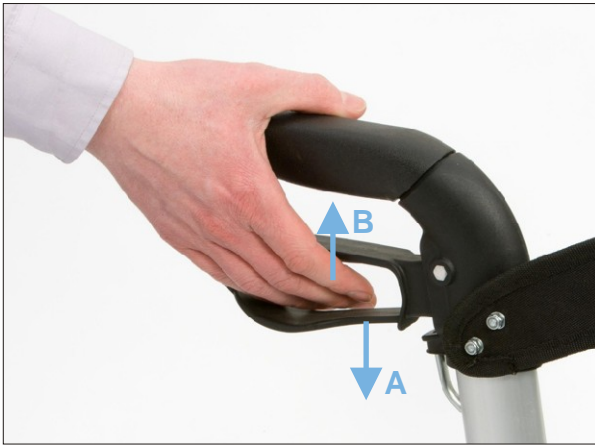

Brake Operation

To use as parking brakes, push down on both brake levers (see "A") and release when the brakes are locked on. To release the brakes, push up on both levers and release.

To use the brake to slow the rollator down, pull up on both brake levers (see "B"). Release the levers to take the brakes off.



Kerb and Obstacle Climbing

To lift up the front wheels of the rollator to help negotiate kerbs and other obstacles, press down on the stepper lever (As shown)

assembly



1. Install the top section of the rollator by pulling upwards on the handles or backrest



2. Lock the handle tubing upright by flipping over the camlock lever

3. Secure the camlock lever by pushing the lever in to the slot (shown).



4. Push down on the cross brace rails until the rails are sat in the plastic receivers.

5. If the bag is required, hook the bag loop over the receiver on both ends of the cross brace rails (as shown)



to fold the rollator

Reverse the previous procedure to fold the rollator (as described below).

1. Remove the bag.
2. Fold the rollator up by pulling up on the strap in the centre of the seat sling (as shown).
3. Release the camlock levers and flip over to allow release handle tubing.
4. Slowly lower the handle tubing to fully fold the rollator.

