


Safety

Do not exceed the maximum user weight, or carry more than one person at a time, as this may cause damage to the wheelchair. It may also cause an injury to the user as the wheelchair can become unstable and therefore unsafe. The wheelchair could tip over.

This wheelchair was designed to be easy to use on even surfaces. Should you come across surfaces with uneven, bumpy or rough ground you are advised to avoid the area, if it is possible to avoid, or to approach slowly and with caution.

If possible it is recommended that you avoid outdoor use during bad weather (such as rain, snow or high wind) as use during bad weather may increase the risk of incidents. Exposure to excess moisture or water may cause rust to some wheelchair components.

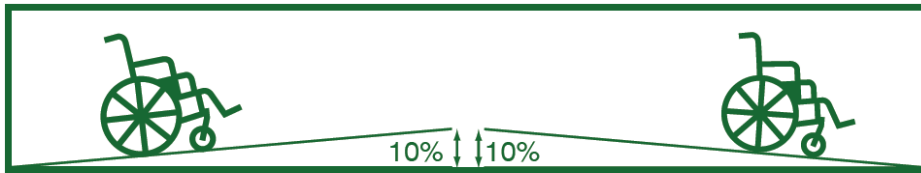

Maximum Safe Incline Angle (Ascending and Descending)

It is recommended that the maximum incline angle to climb with your wheelchair is 10%. Any attempt to climb or descend steeper inclines may cause the wheelchair to become unstable and therefore unsafe. The wheelchair could tip over.

Curbs and other obstacles should be approached with caution and if possible the wheelchair should be driven around them. If these obstacles cannot be avoided it is recommended to approach slowly and at 90° from the front or rear of the wheelchair.

Curb



Correct Curb Approach


Curb



Incorrect Kerb Approach


Assembly Guide (continued)

Step 4




Line up the 2 holes on each foot rest and slide down onto the small pegs above each front wheel.

Step 5



Rotate each foot rest towards the front of the wheelchair until the release lever locks into place.

Step 6



Adjust the length of each footrest by loosening the locking screw. Once the length is adjusted retighten the locking screw.

Storage & Transport

Step 1




To lower the back rest push the levers forward on each side. The wheelchair can be transported with the back rest up or down.

Step 2



Fold the wheelchair by pulling up the handles attached to each side of the seat or by pulling up the front and rear of the seat.

Step 3



To reduce the weight of the wheelchair for transport the foot rests can be completely removed and replaced when needed.